
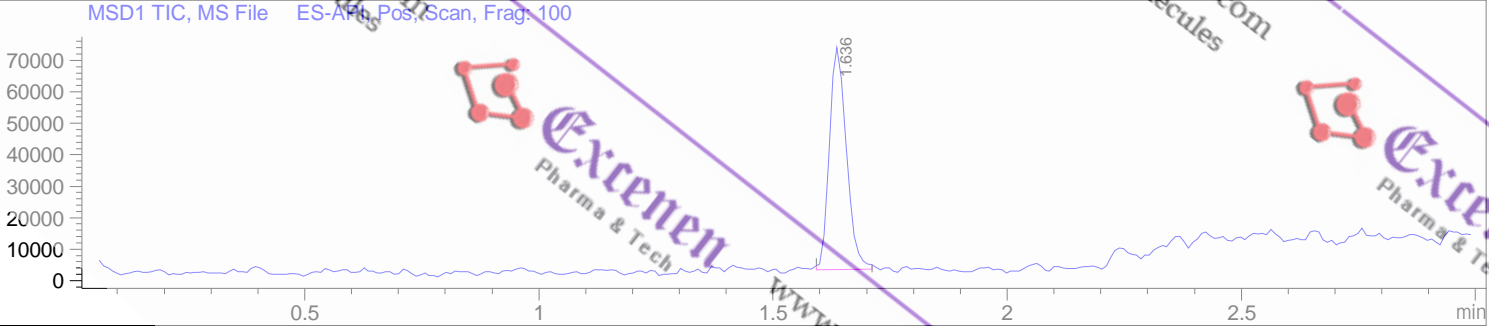
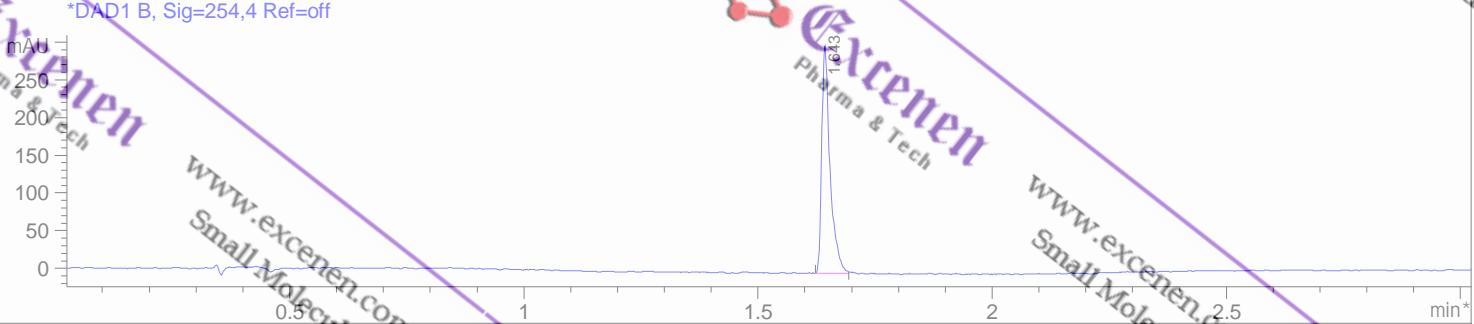


**Analysis Method** : D:\METHODS\1-POS-3MIN.M  
**Sample Info** : Easy-Access Method: '1-POS-3MIN'  
**Method Info** : Mobile Phase: A: water(0.01%TFA) B: ACN(0.01%TFA)  
 Gradient: 5%B increase to 95%B within 1.5 min, 95%B for 1.5 min.  
 Flow Rate: 2.0ml/min  
 Column: Sunfire C18, 4.6\*50mm, 3.5um  
 Column Temperature: 50 C  
 Detection: UV(214,4nm) and MS(ESI,Pos mode,110 to 1500 amu)

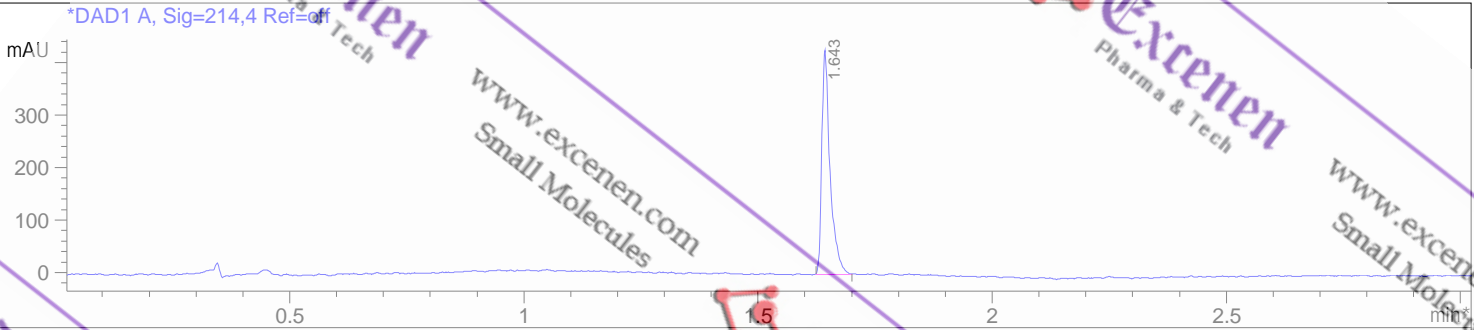

Integration Results for DAD1 A, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%
1.64	0.02	528.67	419.20	100.00

Integration Results for DAD1 B, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%
1.64	0.02	374.25	296.24	100.00

Ret. Time: 1.64

<<<< POSITIVE SPECTRA >>>>

ES-API Positive

